

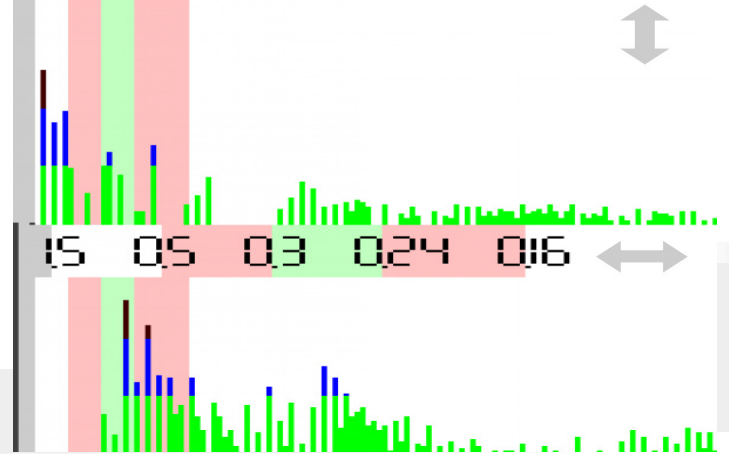
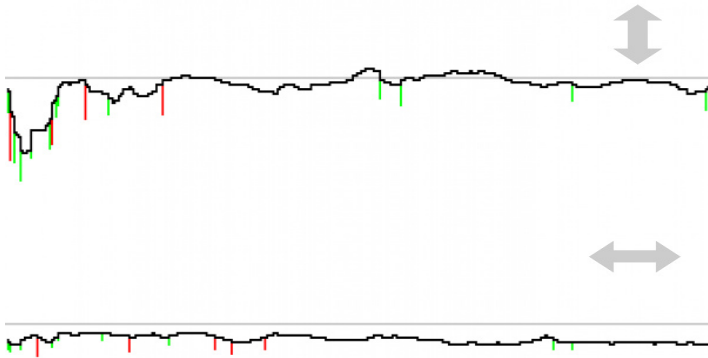


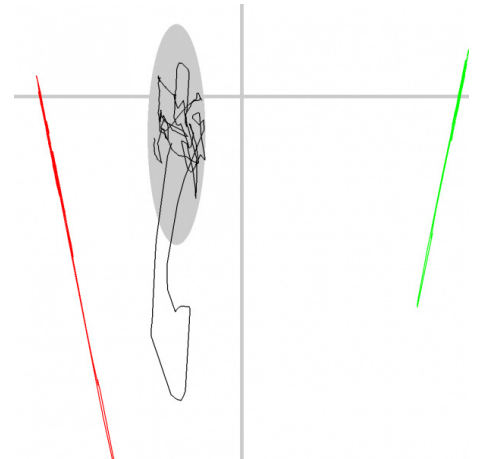

Name _____
Measurement 2015-10-12 19:13
EO - eyes open

Professional stamp

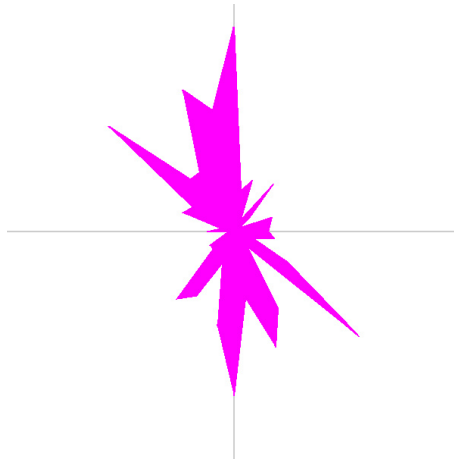

STATIC ANALYSIS

	Left	Right
Forefoot	25% (22)	23% (22)
Backfoot	29% (28)	23% (28)
Lateral side	54% (50)	46% (50)
Front side	48% (44)	52% (56)

DYNAMIC ANALYSIS

	Lateral side	Front side
Mean COP	-5.75 mm	-3.32 mm
Standard deviation	1.27 mm	4.84 mm
Twist	239° (180°)	
Mean speed	0.54 mm/sec	
Area	21.05 cm ² (EO<210, EC<638)	