
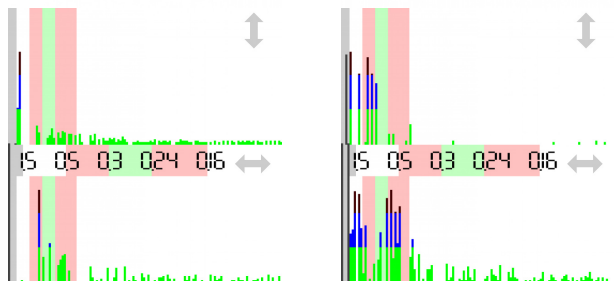
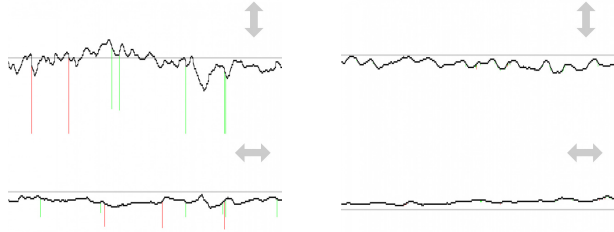


GRAPHICS

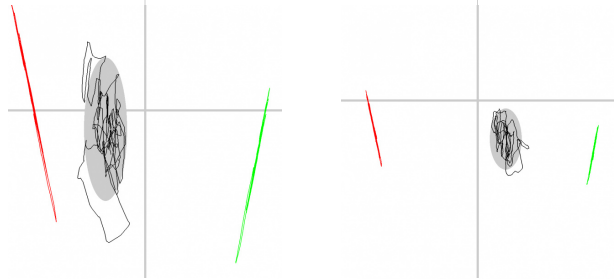

Name _____
 Measurement 2014-08-12 07:56
 ECR - eyes closed retroverted
 Measurement 2015-10-13 07:23
 EO - eyes open

Professional stamp

STATIC ANALYSIS

	Left	Right
Forefoot	27% > 23% (22)	21% < 24% (22)
Backfoot	26% > 25% (28)	25% < 28% (28)
Lateral side	54% > 48% (50)	46% < 52% (50)
	Front	Back
Front side	48% > 47% (50)	52% < 53% (50)

DYNAMIC ANALYSIS

	Lateral side	Front side
Mean COP	-5.80 < 4.09 cm	-2.69 > -5.59 cm
Standard deviation	1.56 > 1.16 cm	5.22 > 2.22 cm
Twist	245.00 > 143.00	° (180°)
Mean speed	0.55 > 0.46	cm/sec
Area	27.77 > 8.83	mm ² (EO<210, EC<638)
Romberg index	314%	(>100%)

Measurement 2014-08-12 07:56

test completo

Measurement 2015-10-13 07:23