



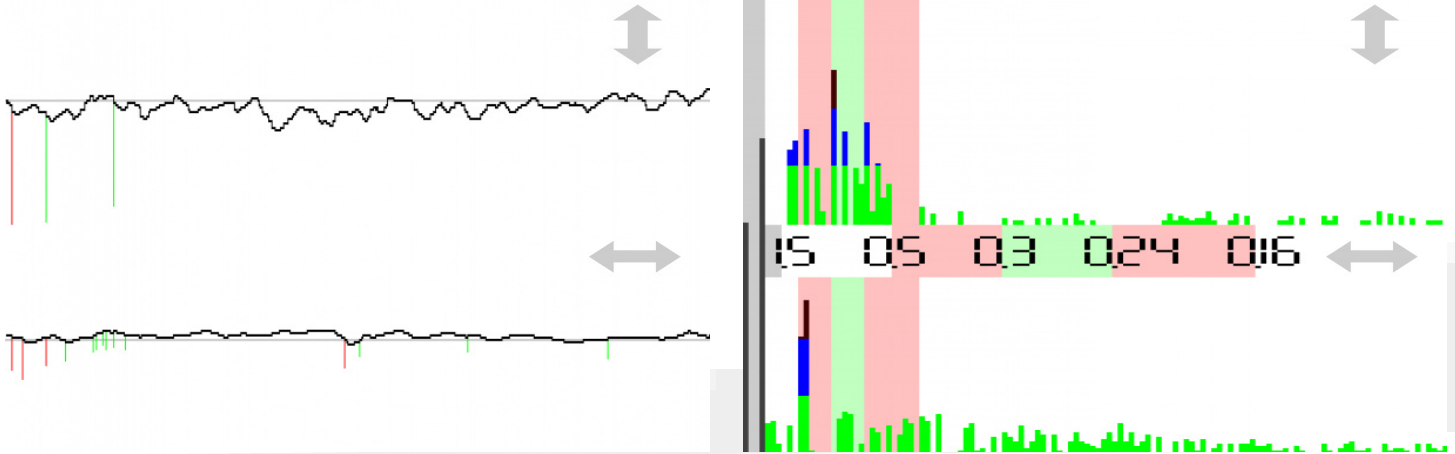

Name _____
Measurement 2014-08-12 07:52
EO - eyes open
test completo

Professional stamp

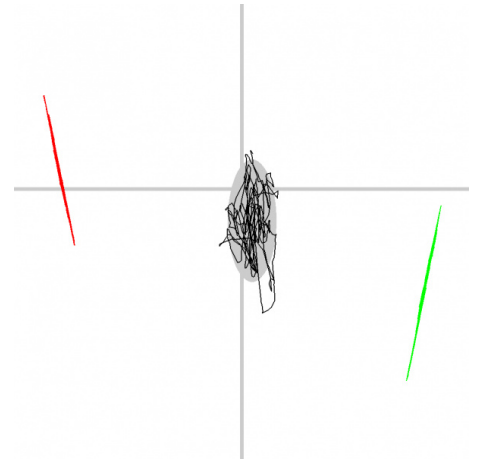

STATIC ANALYSIS

	Left	Right
Forefoot	25% (22)	23% (22)
Backfoot	24% (28)	28% (28)
Lateral side	49% (50)	51% (50)
Front side	Front 48% (44)	Back 52% (56)

DYNAMIC ANALYSIS

	Lateral side	Front side
Mean COP	0.91 mm	-2.76 mm
Standard deviation	1.06 mm	2.69 mm
Twist	161° (180°)	
Mean speed	0.44 mm/sec	
Area	9.72 cm ² (EO<210, EC<638)	