
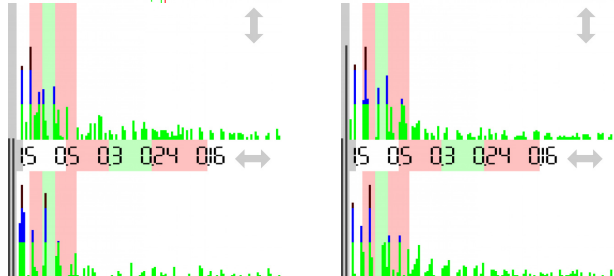
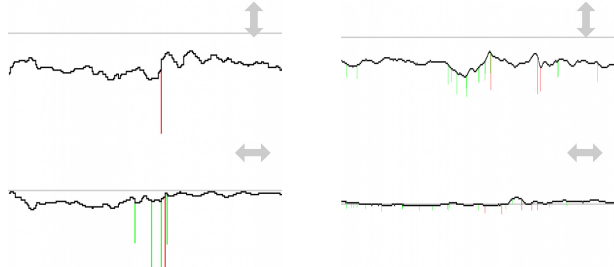
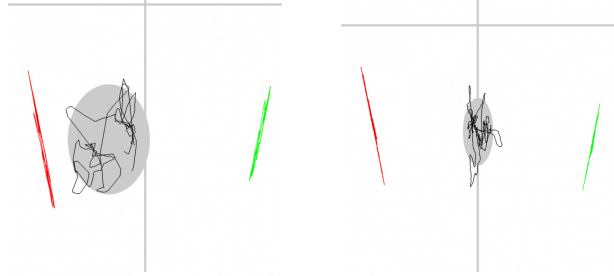
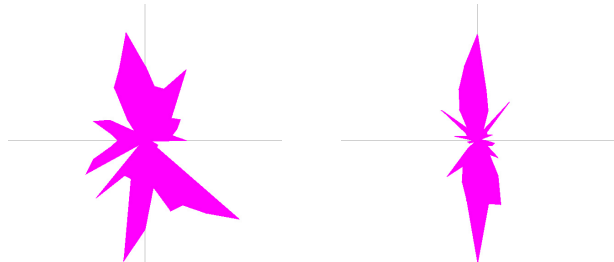


GRAPHICS

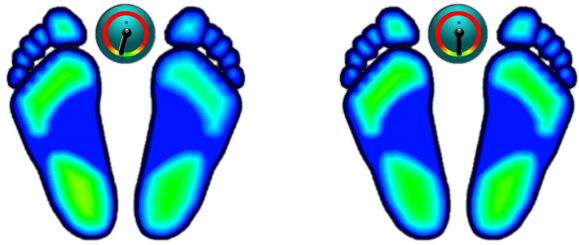

Name _____
 Measurement 2014-06-20 10:04
 ECR - eyes closed retroverted
 Measurement 2016-10-17 00:00
 EO - eyes open

Professional stamp

STATIC ANALYSIS

	Left	Right
Forefoot	20% < 21% (22)	18% < 20% (22)
Backfoot	33% > 29% (28)	29% < 30% (28)
Lateral side	53% > 50% (50)	47% < 50% (50)
	Front	Back
Front side	38% < 41% (50)	62% > 59% (50)

DYNAMIC ANALYSIS

	Lateral side	Front side
Mean COP	-5.28 < 0.05 cm	-19.65 < -15.46 cm
Standard deviation	2.99 > 1.11 cm	4.00 > 2.46 cm
Twist	195.00 > 179.00	° (180°)
Mean speed	0.61 > 0.47	cm/sec
Area	40.81 > 9.34	mm ² (EO<210, EC<638)
Romberg index	436%	(>100%)

Measurement 2014-06-20 10:04

?test

Measurement 2016-10-17 00:00

cellulare in mano