
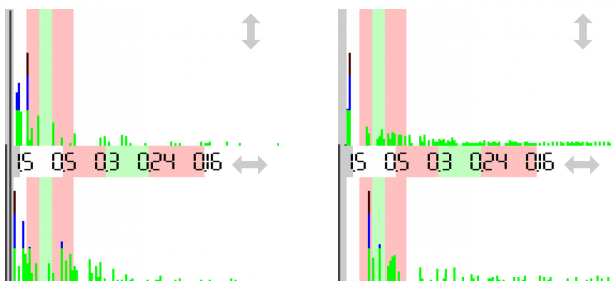
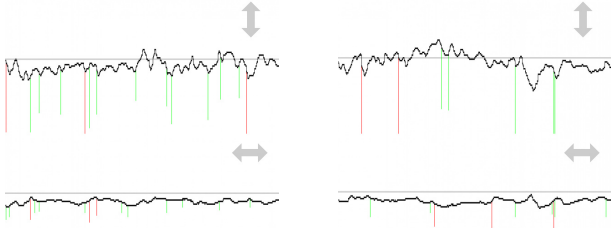
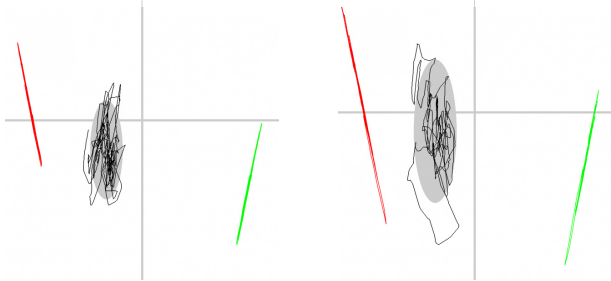


GRAPHICS

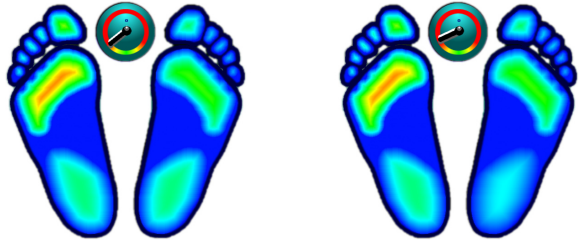

Name _____
 Measurement 2014-08-12 07:54
 EC - eyes closed
 Measurement 2014-08-12 07:56
 ECR - eyes closed retroverted

Professional stamp

STATIC ANALYSIS

	Left	Right
Forefoot	27% = 27% (22)	21% = 21% (22)
Backfoot	26% = 26% (28)	26% > 25% (28)
Lateral side	53% < 54% (50)	47% > 46% (50)
	Front	Back
Front side	47% < 48% (50)	53% > 52% (50)

DYNAMIC ANALYSIS

	Lateral side	Front side
Mean COP	-5.24 > -5.80 cm	-4.28 < -2.69 cm
Standard deviation	1.19 < 1.56 cm	3.61 < 5.22 cm
Twist	230.00 < 245.00	° (180°)
Mean speed	0.63 > 0.55	cm/sec
Area	14.73 < 27.77	mm ² (EO<210, EC<638)
Romberg index	53%	(>100%)

Measurement 2014-08-12 07:54

test completo

Measurement 2014-08-12 07:56

test completo