

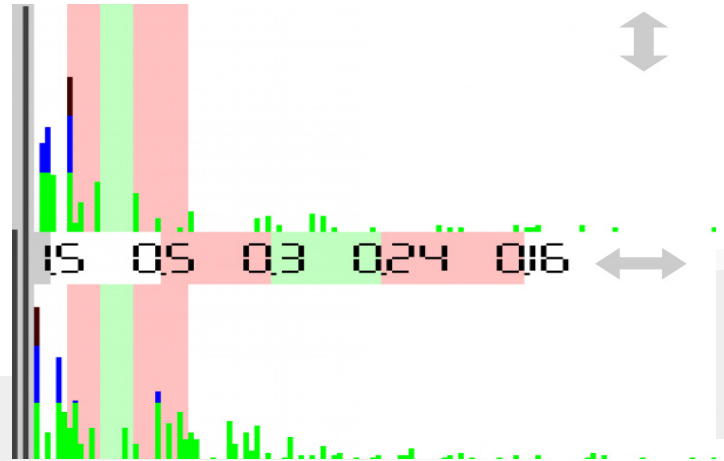
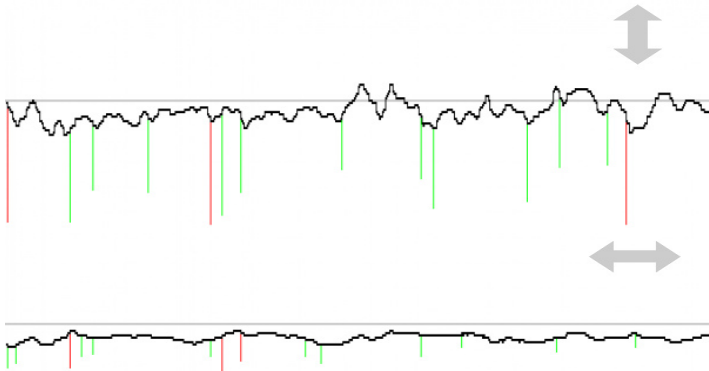


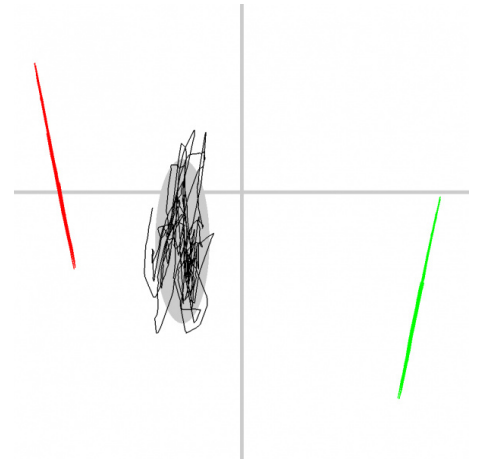

Name _____
 Measurement 2014-08-12 07:54
 EC - eyes closed
 test completo

Professional stamp

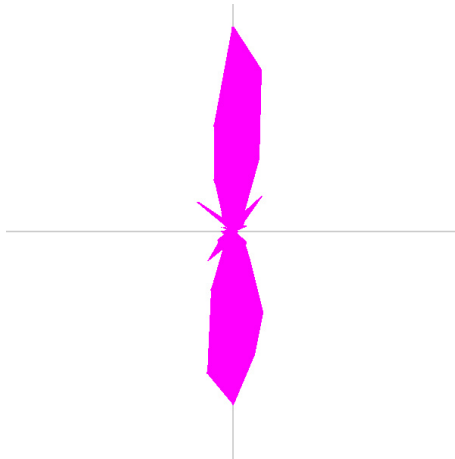

STATIC ANALYSIS

	Left	Right
Forefoot	27% (22)	21% (22)
Backfoot	26% (28)	26% (28)
Lateral side	53% (50)	47% (50)
Front side	47% (44)	53% (56)

DYNAMIC ANALYSIS

	Lateral side	Front side
Mean COP	-5.24 mm	-4.28 mm
Standard deviation	1.19 mm	3.61 mm
Twist	230° (180°)	
Mean speed	0.63 mm/sec	
Area	14.73 cm ² (EO<210, EC<638)	