







Name \_\_\_\_\_

Measurement 2016-10-18 19:41

EO - eyes open

Professional stamp

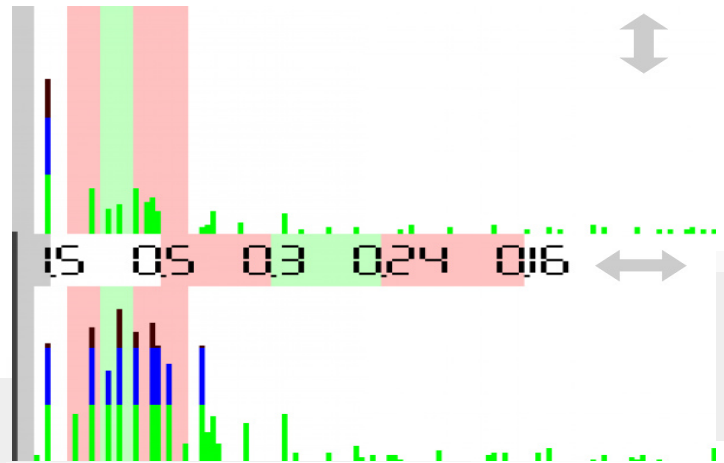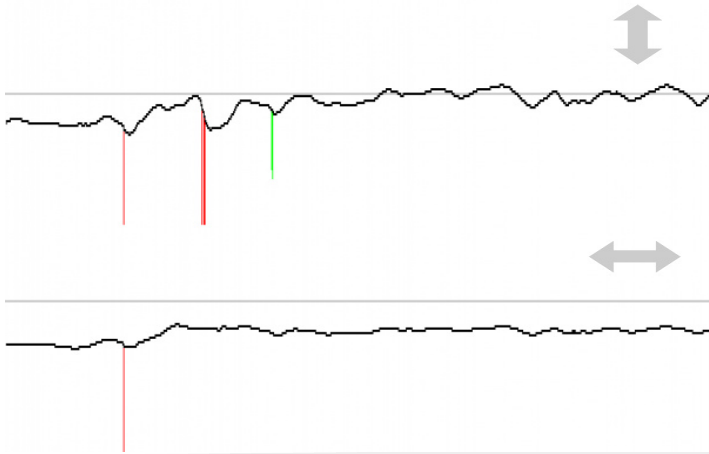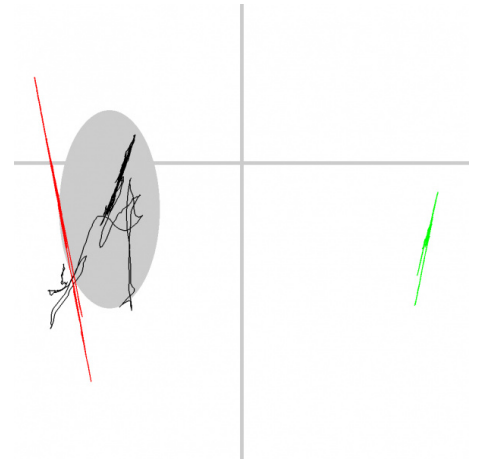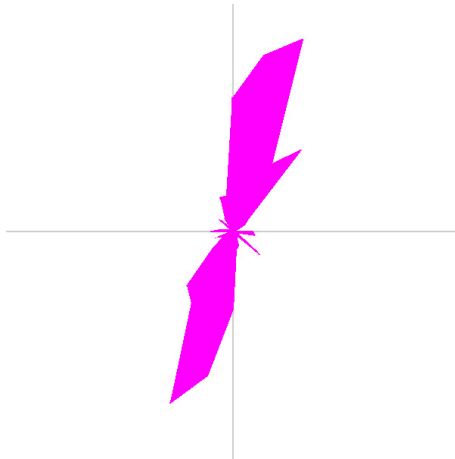

**STATIC ANALYSIS**

	<b>Left</b>	<b>Right</b>
Forefoot	33% (22)	10% (22)
Backfoot	38% (28)	20% (28)
Lateral side	71% (50)	29% (50)
	<b>Front</b>	<b>Back</b>
Front side	43% (44)	57% (56)

**DYNAMIC ANALYSIS**

	<b>Lateral side</b>	<b>Front side</b>
Mean COP	-11.62 mm	-4.03 mm
Standard deviation	2.2 mm	4.34 mm
Twist	250° (180°)	
Mean speed	0.57 mm/sec	
Area	32.53 cm <sup>2</sup> (EO<210, EC<638)	

StabilApp - WARNING! These are just a postural and functional analysis.  
 Diagnosis and treatment are carried out by a medical specialist.  
 © 2014-2024 Rodolfo Zarli