
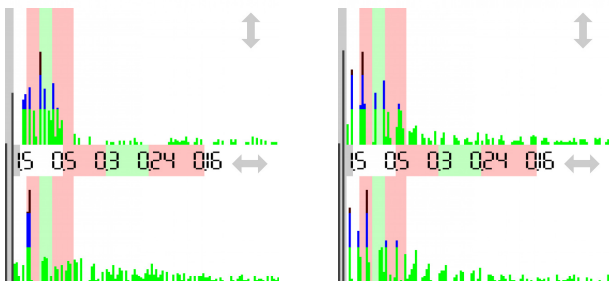
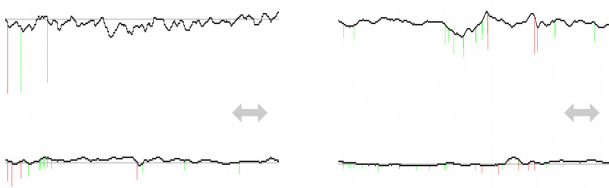
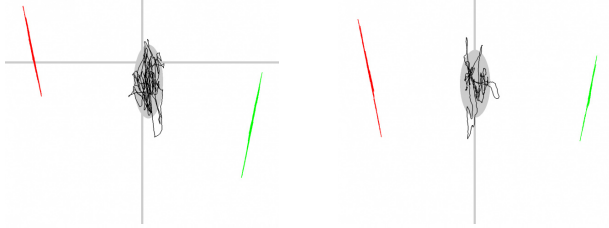


GRAPHICS

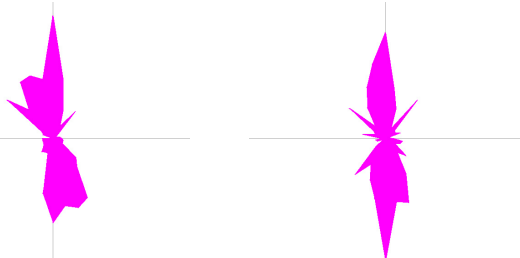

Name _____
 Measurement 2014-08-12 07:52
 EO - eyes open
 Measurement 2016-10-17 00:00
 EO - eyes open

Professional stamp

STATIC ANALYSIS

	Left	Right
Forefoot	25% > 21% (22)	23% > 20% (22)
Backfoot	24% < 29% (28)	28% < 30% (28)
Lateral side	49% < 50% (50)	51% > 50% (50)
	Front	Back
Front side	48% > 41% (50)	52% < 59% (50)

DYNAMIC ANALYSIS

	Lateral side	Front side
Mean COP	0.91 > 0.05 cm	-2.76 > -15.46 cm
Standard deviation	1.06 < 1.11 cm	2.69 > 2.46 cm
Twist	161.00 < 179.00	° (180°)
Mean speed	0.44 < 0.47	cm/sec
Area	9.72 > 9.34	mm ² (EO<210, EC<638)
Romberg index	104%	(>100%)

Measurement 2014-08-12 07:52

test completo

Measurement 2016-10-17 00:00

cellulare in mano