
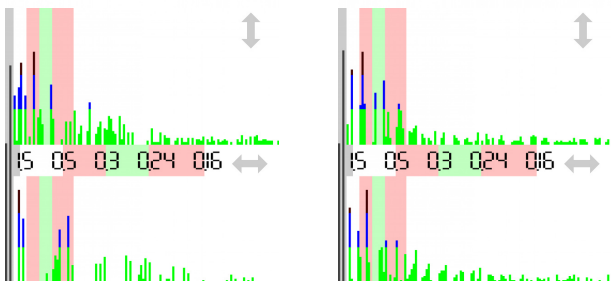
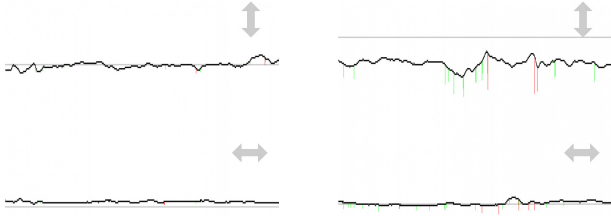
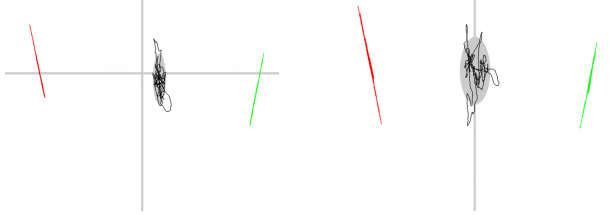


**GRAPHICS**

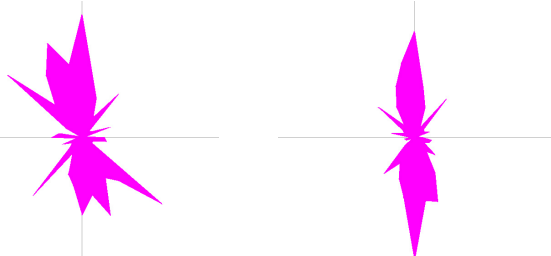

Name \_\_\_\_\_  
 Measurement 2015-10-13 07:16  
 EO - eyes open  
 Measurement 2016-10-17 00:00  
 EO - eyes open

Professional stamp

**STATIC ANALYSIS**

	Left	Right
Forefoot	25% > 21% (22)	25% > 20% (22)
Backfoot	24% < 29% (28)	26% < 30% (28)
Lateral side	49% < 50% (50)	51% > 50% (50)
Front side	50% > 41% (50)	50% < 59% (50)

**DYNAMIC ANALYSIS**

	Lateral side	Front side
Mean COP	2.51 > 0.05 cm	-0.75 > -15.46 cm
Standard deviation	0.47 < 1.11 cm	1.85 < 2.46 cm
Twist	106.00 < 179.00	° (180°)
Mean speed	0.34 < 0.47	cm/sec
Area	2.98 < 9.34	mm <sup>2</sup> (EO<210, EC<638)
Romberg index	31%	(>100%)

Measurement 2015-10-13 07:16

Measurement 2016-10-17 00:00

cellulare in mano