


GRAPHICS

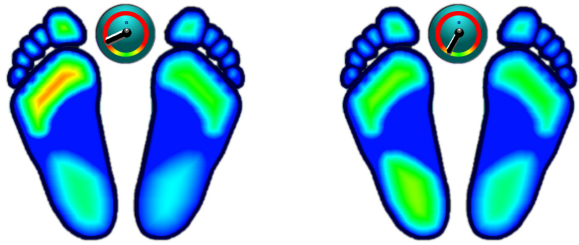

Name _____
 Measurement 2014-08-12 07:56
 ECR - eyes closed retroverted
 Measurement 2016-12-31 06:30
 EO - eyes open


Professional stamp

STATIC ANALYSIS

	Left	Right
Forefoot	27% > 22% (22)	21% > 18% (22)
Backfoot	26% < 33% (28)	25% < 26% (28)
Lateral side	54% < 56% (50)	46% > 44% (50)
Front side	48% > 40% (50)	52% < 60% (50)

DYNAMIC ANALYSIS

	Lateral side	Front side
Mean COP	-5.80 > -9.11 cm	-2.69 > -15.85 cm
Standard deviation	1.56 < 2.72 cm	5.22 > 4.36 cm
Twist	245.00 > 209.00	° (180°)
Mean speed	0.55 > 0.54	cm/sec
Area	27.77 < 40.42	mm ² (EO<210, EC<638)
Romberg index	68%	(>100%)

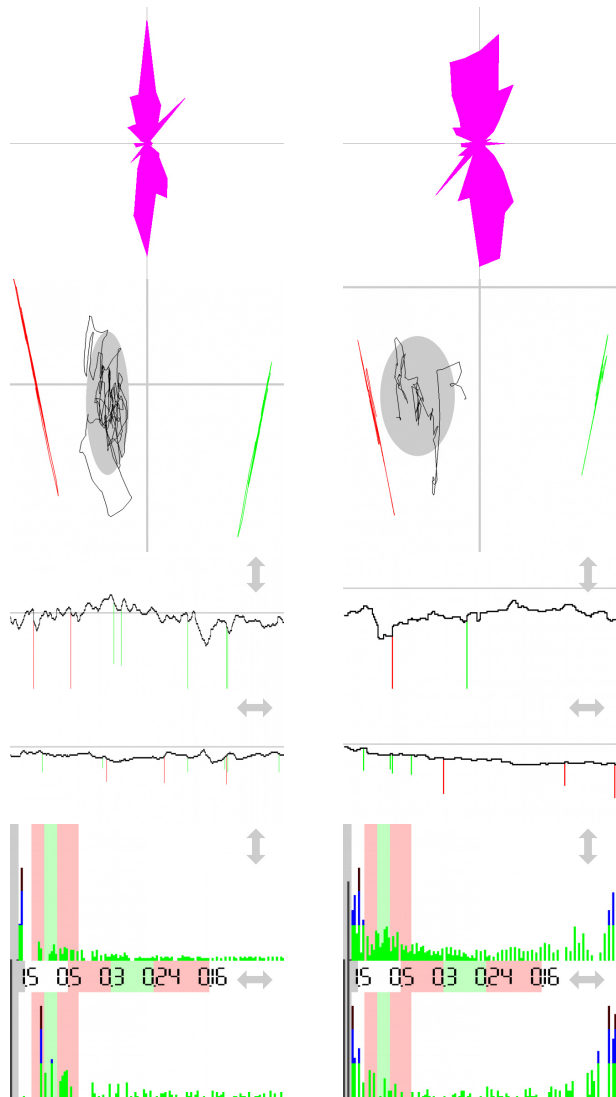

Measurement 2014-08-12 07:56

test completo

Measurement 2016-12-31 06:30