

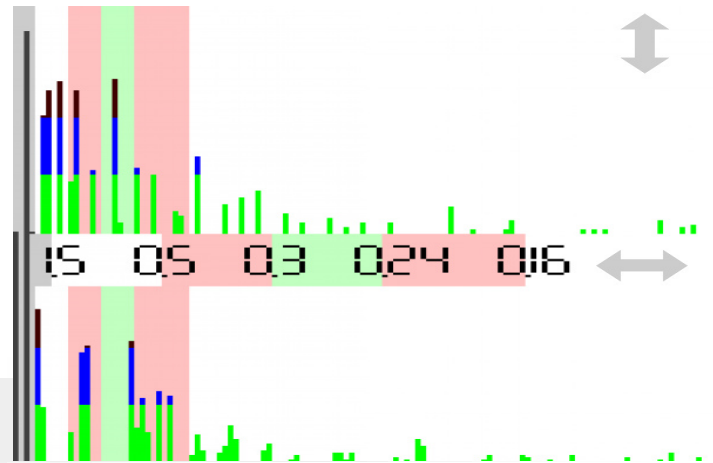
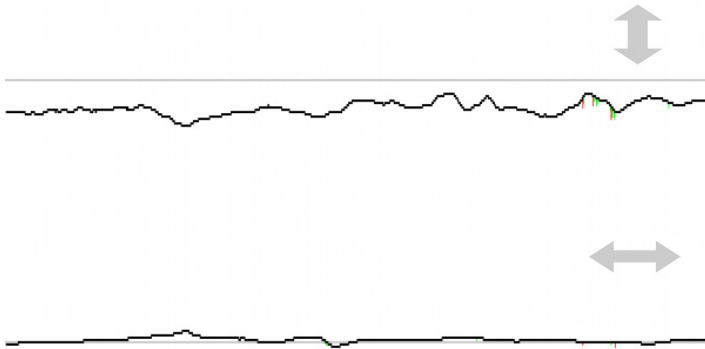


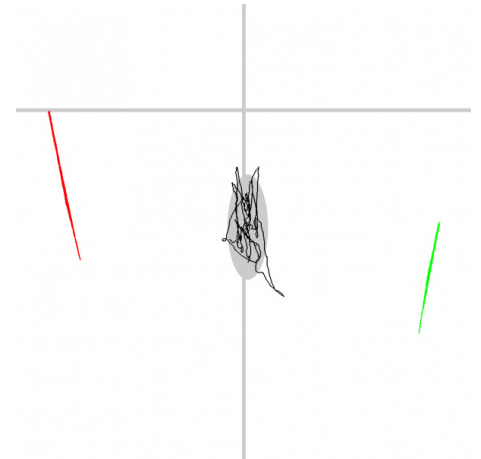

Name \_\_\_\_\_  
 Measurement 2015-10-13 07:28  
 EO - eyes open

Professional stamp

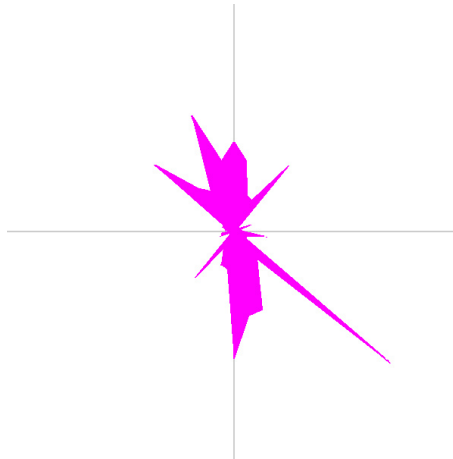

### STATIC ANALYSIS

	Left	Right
Forefoot	23% (22)	21% (22)
Backfoot	27% (28)	29% (28)
Lateral side	50% (50)	50% (50)
Front side	44% (44)	56% (56)

### DYNAMIC ANALYSIS

	Lateral side	Front side
Mean COP	0.34 mm	-10.24 mm
Standard deviation	0.89 mm	2.3 mm
Twist	178° (180°)	
Mean speed	0.39 mm/sec	
Area	6.98 cm <sup>2</sup> (EO<210, EC<638)	