
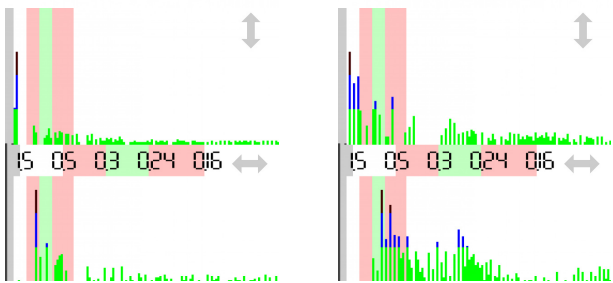
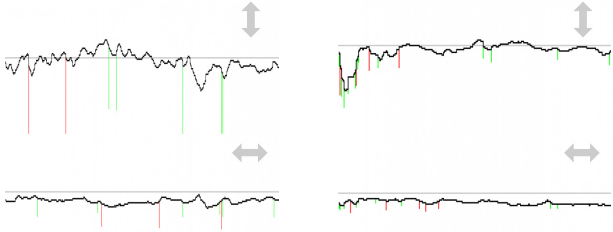
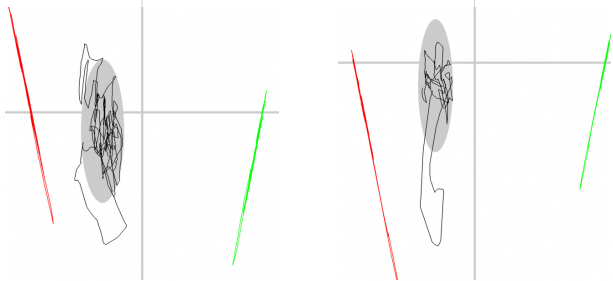


GRAPHICS

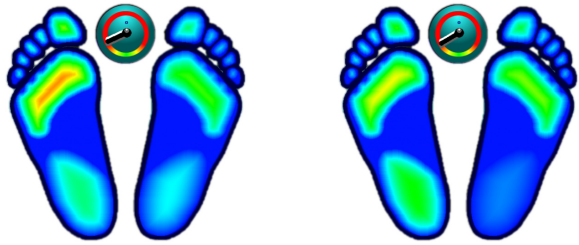

Name _____
 Measurement 2014-08-12 07:56
 ECR - eyes closed retroverted
 Measurement 2015-10-12 19:13
 EO - eyes open

Professional stamp

STATIC ANALYSIS

	Left	Right
Forefoot	27% > 25% (22)	21% < 23% (22)
Backfoot	26% < 29% (28)	25% > 23% (28)
Lateral side	54% = 54% (50)	46% = 46% (50)
Front side	Front 48% = 48% (50)	Back 52% = 52% (50)

DYNAMIC ANALYSIS

	Lateral side	Front side
Mean COP	-5.80 < -5.75 cm	-2.69 > -3.32 cm
Standard deviation	1.56 > 1.27 cm	5.22 > 4.84 cm
Twist	245.00 > 239.00	° (180°)
Mean speed	0.55 > 0.54	cm/sec
Area	27.77 > 21.05	mm ² (EO<210, EC<638)
Romberg index	131%	(>100%)

Measurement 2014-08-12 07:56

test completo

Measurement 2015-10-12 19:13